

All data taken at the Pacific Northwest National Laboratory

FTS Operators: John S. Loring

Data Analysis: Russell G. Tonkyn

Composite spectrum for: Acetone

- First Column: Position in wavenumber (cm^{-1})
- Second column: Real refractive index $n(\tilde{\nu})$ (dispersion index)
- Third column: Imaginary refractive index, $k(\tilde{\nu})$ (absorption index per unit length in centimeters)

Where the complex refractive index $\hat{n} = n(\tilde{\nu}) + ik(\tilde{\nu})$

Following Bertie (in the references below) we define the absorbance as $A = -\log_{10}(I/I_0)$ and the linear absorption coefficient $K = A/d$, where d is the path length. The connection between the imaginary refractive index and the absorbance coefficient arises from the following: $2.303K = 4\pi\tilde{\nu}k$

See the following references for a detailed description of terms and units:

- 1) Bertie, J. E., Zhang, S. L., Eysel, H. H., Baluja, S., & Ahmed, M. K. (1993). Infrared Intensities of Liquids XI: Infrared Refractive Indices from 8000 to 2 cm^{-1} , Absolute Integrated Intensities, and Dipole Moment Derivatives of Methanol at 25°C . *Appl. Spec.*, 47(8), 1100-1114 doi:10.1366/0003702934067973
- 2) Bertie, J. E., Zhang, S. L., & Keefe, C. D. (1995). Measurement and use of absolute infrared absorption intensities of neat liquids. *Vibrational Spectroscopy*, 8(2), 215-229. doi:10.1016/0924-2031(94)00038-i

Sample:

- Chemical name, formula and CAS number: Acetone, $\text{C}_3\text{H}_6\text{O}$, [67-64-1]
- IUPAC name: Propan-2-one
- Synonyms: 2-Propanone; β -Ketopropane; Dimethyl ketone; Dimethylformaldehyde; Methyl ketone
- Physical properties: FW = 58.08 g/mole; mp = -94.7°C ; bp = 56.05°C ; $\rho = 0.7845\text{ g/cm}^3$
- Supplier and stated purity: Alfa Aesar, 99+% (Lot # U07E003)
- Temperature of sample: 26°C ($\pm 1^\circ\text{C}$)
- Individual samples were measured at the following path lengths: MIR: 4.21, 4.35, 8.08, 10.8, 11.0, 15.8, 35.9, 56.0, 110, 204 and 507 μm ; NIR: 109, 204, 507, 994 and 2186 μm . Final data are a composite of these spectra.
- Sample cell window material is potassium bromide (KBr) except the 11.0 (MIR), 110 (MIR), 507 (MIR), 109 (NIR), 507 (NIR) and 994 (NIR) cell windows were potassium chloride (KCl).
- Preparation: None.

NIR Instrument Parameters:

- Bruker Vertex 70, purged with UHP nitrogen
- Spectral range: 10,000 to $3,000\text{ cm}^{-1}$ (1.0 to 3.33 microns)
- NIR source: Quartz tungsten bulb
- Beamsplitter: Broadband Potassium bromide (KBr)
- Detector: DLTGS at room temperature
- Aperture: 3 mm
- Folding limits: 31601 to 0 cm^{-1}

MIR Instrument Parameters:

- Bruker Vertex 70, purged with UHP nitrogen
- Spectral range: 7800 to 400 cm^{-1} (1.282 to 25 microns)
- IR source: Silicon carbide glow bar
- Beamsplitter: Broadband Potassium bromide (KBr)
- Detector: DLTGS at room temperature
- Aperture: 3 mm
- Folding limits: 15802 to 0 cm^{-1}

NIR/MIR Instrument Parameters:

- Instrument resolution: 2.0 cm^{-1}
- Number of interferograms averaged per single channel spectrum: 128
- Apodization: Norton-Beer, Medium
- Phase correction: Mertz
- Scanner velocity: 10 kHz
- Interferogram zerofill: 4x
- Spectral interval after zerofilling: 0.4823 cm^{-1}

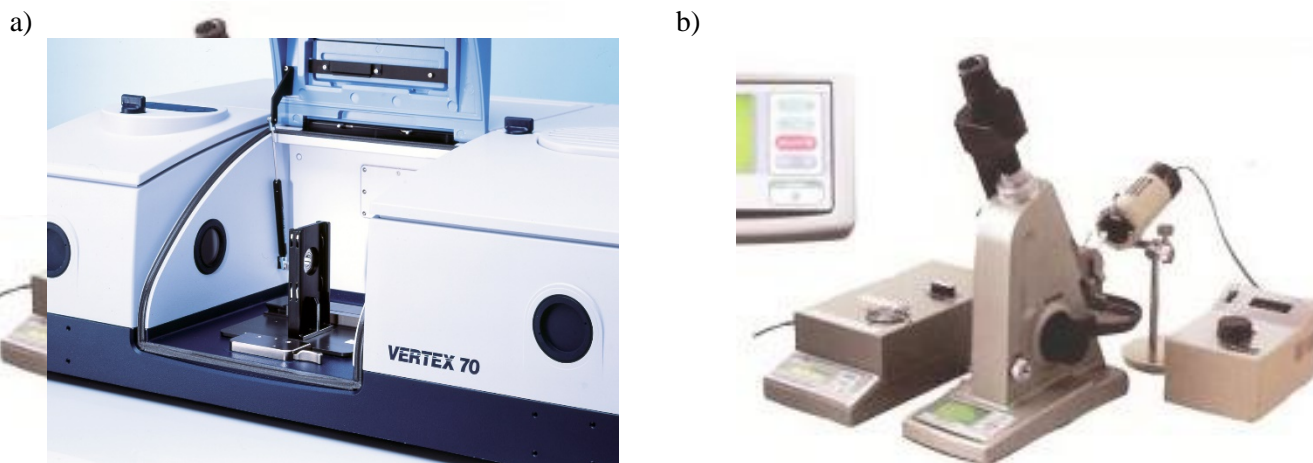


Figure 1: The Bruker Vertex 70 FTIR (a) and Abbe refractometer (b).

Measured Refractive Index:

The refractive index for Acetone was measured at $8\text{ }^{\circ}\text{C}$ using an Atago model DR-M2/1550 Abbe refractometer. Notch filters were employed in front of a white light source to make measurements at multiple wavelengths. An infrared viewer from Atago was used to detect signal at 1550 nm . The temperature was controlled to match that in the sample compartment of the FTIR using a heated circulating bath.

| | | |
|-----------------------|----------------------|----------------------|
| 480 nm: $n = 1.3714$ | 486 nm: $n = 1.3708$ | 546 nm: $n = 1.3672$ |
| 589 nm: $n = 1.3655$ | 644 nm: $n = 1.3636$ | 656 nm: $n = 1.3634$ |
| 1550 nm: $n = 1.3464$ | | |

The refractive index, n , vs. wavelength in microns, λ , was fit to an equation similar to that of Sellmeier:

$$n(\lambda) = \{a + b/(\lambda^2 - c)\}^{1/2}$$

The resulting best-fit equation was used to find the refractive index at the highest energy data points in our experimental spectra. After extrapolation, the $n(7800\text{ cm}^{-1})$ and $n(10,000\text{ cm}^{-1})$ results were corrected for a $19\text{ }^{\circ}\text{C}$ increase in temperature to match the FTIR measurements by using an estimate of -0.00045 per degree ($19\text{ }^{\circ}\text{C}$ difference is equal to a decrease in value by 0.0089). For Acetone, the results were

$$\begin{aligned} n(7800\text{ cm}^{-1}) &= 1.340\text{ at } 27\text{ }^{\circ}\text{C} \text{ (1.3489 at } 8\text{ }^{\circ}\text{C) for MIR data and} \\ n(10,000\text{ cm}^{-1}) &= 1.345\text{ at } 27\text{ }^{\circ}\text{C} \text{ (1.3532 at } 8\text{ }^{\circ}\text{C) for NIR and merged data.} \end{aligned}$$

Post Processing and Related Parameters:

For the MIR, a composite spectrum was created from 11 absorbance spectra (base-10) taken at 11 path lengths: 4.21, 4.35, 8.08, 10.8, 11.0, 15.8, 35.9, 56.0, 110, 204 and 507 micrometers (μm). For the NIR, a composite spectrum was created from 5 absorbance spectra (base-10) taken at 5 path lengths: 109, 204, 507, 994 and 2186 μm . The same cells for the 100, 200 and 500 μm path lengths were used for both spectral ranges. At each path length several spectra were measured and the results averaged for better signal to noise. The measured cell lengths were adjusted using Beer's law plots in which the NIR and MIR data were analyzed independently.

- 1) The imaginary part of the refractive index, or k vector, was determined for each absorbance file as per Bertie's program "RNJ46A" (see reference above). This takes into account the reflective losses due to the KBr windows and the measured refractive index at 7800 cm^{-1} for the MIR data and $10,000\text{ cm}^{-1}$ for the NIR data.
- 2) A composite k vector is created via a classical, weighted, linear, least squares fit using the output files of program "RNJ46A": Intercept=0, slope is fitted, individual absorbance values weighted by T^2 (transmission squared), all absorbance values ≥ 2.5 are given zero weight. For the MIR, six composite vectors were created and merged by hand.
 - a) The first k vector used the results from the 110 through 507 μm cells. This k vector determined the final values for the range from 7800 to 4600 cm^{-1} .
 - b) The second k vector used the results from the 35.9 through 507 μm cells. This k vector determined the final values for the range from 4600 to 3300 cm^{-1} .
 - c) The third k vector used the results from the 10.8 through 204 (not including 11.02 and 15.8) μm cells. This k vector determined the final values for the range from 3300 to 2600 cm^{-1} .
 - d) The fourth k vector used the results from the 56.0 through 507 μm cells. This k vector determined the final values for the range from 2600 to 1925 cm^{-1} .
 - e) The fifth k vector used the results from the 4.21 through 56.0 μm cells. This k vector determined the final values for the range from 1925 to 650 cm^{-1} .
 - f) The sixth k vector used the results from the 4.21 through 8.08 and 11.0 through 56.0 (not including 10.82) μm cells. This k vector determined the final values for the range from 650 to 400 cm^{-1} .
- 3) A frequency correction was applied to the resulting composite MIR k vector.
 - a) Frequency correction (already applied): $\tilde{\nu}(\text{corrected}) = [\tilde{\nu}(\text{instrument}) * 0.999869 + 0.0158818]$ as determined by comparing measured atmospheric spectral lines (H_2O and CO_2) to values from the Northwest Infrared Spectral Library Database.
- 4) For the NIR, two composite vectors were created and merged by hand.
 - a) The first k vector used the results from the 994 and 2186 μm cells. This k vector determined the final values for the range from 10000 to 6300 cm^{-1} .
 - b) The second k vector used the results from the 110 through 2186 μm cells. This k vector determined the final values for the range from 6300 to 400 cm^{-1} .
- 5) A frequency correction was applied to the resulting composite NIR k vector.
 - a) Frequency correction (already applied): $\tilde{\nu}(\text{corrected}) = [\tilde{\nu}(\text{instrument}) * 0.999869 + 0.0158818]$ as determined by comparing measured atmospheric spectral lines (H_2O and CO_2) to values from the Northwest Infrared Spectral Library Database.
- 6) Finally, the MIR data were mapped onto the NIR x-axis using an interpolation routine, i.e. the Make Compatible command in OPUS 5.5. Then the composite MIR and NIR k vectors were merged to generate a final composite k vector across the entire spectral range. The NIR data were used exclusively above 5000 cm^{-1} , and only the MIR data were used below 4500 cm^{-1} . A weighted average, with the weight of the MIR vector increasing linearly from 0 to 100% between 5000 and 4500 cm^{-1} was used in the overlapping spectral region. The resulting composite k vector and the refractive index at $10,000\text{ cm}^{-1}$ were used to create the final n vector using the Kramers-Kronig relation, as per Bertie's program "LZZKTB."

Photograph of Sample Acetone:

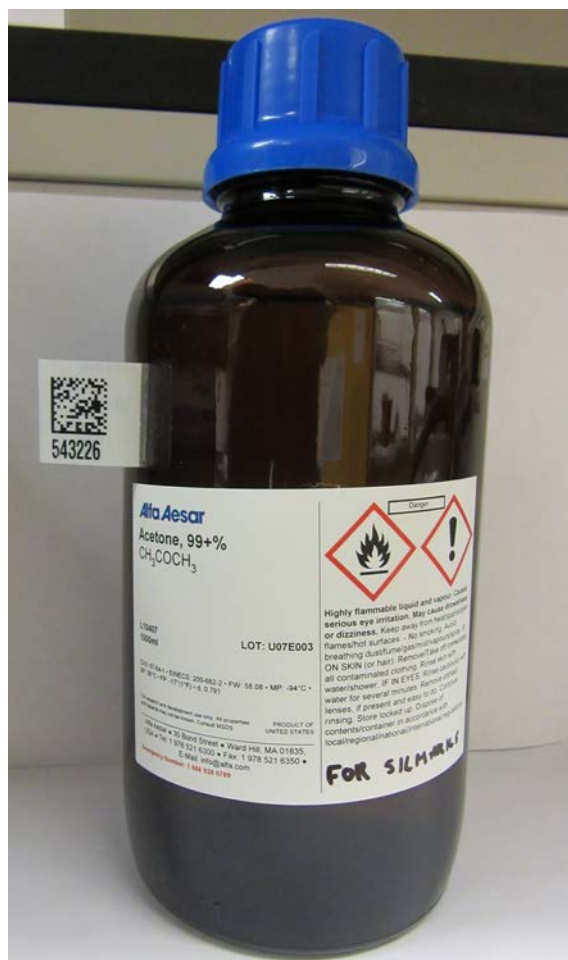


Figure 2: Acetone in Alfa Aesar container.