

All data taken at the Pacific Northwest National Laboratory  
FTS Operators: Ashley M. Oeck  
Data Analysis: Russell G. Tonkyn

**Composite spectrum for: Tetraglyme**

- First Column: Position in wavenumber ( $\text{cm}^{-1}$ )
- Second column: Real refractive index  $n(\tilde{\nu})$  (dispersion index)
- Third column: Imaginary refractive index,  $k(\tilde{\nu})$  (absorption index per unit length in centimeters)

Where the complex refractive index  $\hat{n} = n(\tilde{\nu}) + ik(\tilde{\nu})$

Following Bertie (in the references below) we define the absorbance as  $A = -\log_{10}(I/I_0)$  and the linear absorption coefficient  $K = A/d$ , where  $d$  is the path length. The connection between the imaginary refractive index and the absorbance coefficient arises from the following:  $2.303K = 4\pi\tilde{\nu}k$

See the following references for a detailed description of terms and units:

- 1) Bertie, J. E., Zhang, S. L., Eysel, H. H., Baluja, S., & Ahmed, M. K. (1993). Infrared Intensities of Liquids XI: Infrared Refractive Indices from 8000 to  $2\text{ cm}^{-1}$ , Absolute Integrated Intensities, and Dipole Moment Derivatives of Methanol at  $25^\circ\text{C}$ . *Appl. Spec.*, 47(8), 1100-1114 doi:10.1366/0003702934067973
- 2) Bertie, J. E., Zhang, S. L., & Keefe, C. D. (1995). Measurement and use of absolute infrared absorption intensities of neat liquids. *Vibrational Spectroscopy*, 8(2), 215-229. doi:10.1016/0924-2031(94)00038-i

**Sample:**

- Chemical name, formula and CAS number: Tetraglyme,  $\text{C}_{10}\text{H}_{22}\text{O}_5$ , [143-24-8]
- IUPAC name: 2,5,8,11,14-Pentaoxapentadecane
- Synonyms: Tetraethylene glycol dimethyl ether; Bis[2-(2-methoxyethoxy)ethyl] ether; Dimethoxytetraethylene glycol; Dimethyltetraglycol; TEGDME
- Physical properties: FW = 222.28 g/mole; mp =  $-30^\circ\text{C}$ ; bp =  $275\text{--}276^\circ\text{C}$ ;  $\rho = 1.009\text{ g/cm}^3$
- Supplier and stated purity: Aldrich,  $\geq 99\%$  (Lot # BCBV4743)
- Temperature of sample:  $26^\circ\text{C}$  ( $\pm 1^\circ\text{C}$ )
- Individual samples were measured at the following path lengths: MIR: 3.70, 7.21, 19.8, 41.8, 112, 198 and  $502\text{ }\mu\text{m}$ ; NIR: 113, 200, 504, 990 and  $3054\text{ }\mu\text{m}$ . Final data are a composite of these spectra.
- Sample cell window material is potassium bromide (KBr) except for 3.70, 41.8 and  $502\text{ }\mu\text{m}$  cells, which are potassium chloride (KCl).
- Preparation: None.

**NIR Instrument Parameters:**

- Tensor 37, purged with UHP nitrogen
- Spectral range:  $10,000\text{ to }3,000\text{ cm}^{-1}$  (1.0 to 3.33 microns)
- NIR source: Quartz tungsten bulb
- Beamsplitter: Calcium fluoride ( $\text{CaF}_2$ )
- Detector: DLTGS at room temperature
- Aperture: 3 mm
- Folding limits:  $15800\text{ to }0\text{ cm}^{-1}$


**MIR Instrument Parameters:**

- Tensor 27, purged with UHP nitrogen
- Spectral range:  $7800\text{ to }400\text{ cm}^{-1}$  (1.282 to 25 microns)
- IR source: Silicon carbide glow bar
- Beamsplitter: Broadband Potassium bromide (KBr)
- Detector: DLTGS at room temperature
- Aperture: 3 mm
- Folding limits:  $15801\text{ to }0\text{ cm}^{-1}$

### NIR/MIR Instrument Parameters:

- Instrument resolution:  $2.0\text{ cm}^{-1}$
- Number of interferograms averaged per single channel spectrum: 128
- Apodization: Norton-Beer, Medium
- Phase correction: Mertz
- Scanner velocity: 10 kHz
- Interferogram zerofill: 4x
- Spectral interval after zerofilling:  $0.4823\text{ cm}^{-1}$

a)

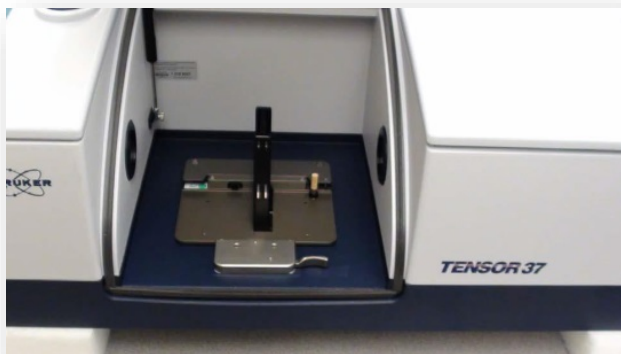

b)



Figure 1: The Bruker Tensor 37 FTIR (a) and Tensor 27 FTIR (b).

### Measured Refractive Index:

The refractive index for Tetraglyme was measured at  $25\text{ }^{\circ}\text{C}$  using an Atago model DR-M2/1550 Abbe refractometer. Notch filters were employed in front of a white light source to make measurements at multiple wavelengths. An infrared viewer from Atago was used to detect signal at  $1550\text{ nm}$ . The temperature was controlled to match that in the sample compartment of the FTIR using a heated circulating bath.

480 nm:	$n = 1.4363$	486 nm:	$n = 1.436$	546 nm:	$n = 1.4318$
589 nm:	$n = 1.4299$	644 nm:	$n = 1.4283$	656 nm:	$n = 1.4277$
1550 nm:	$n = 1.4117$				

The refractive index,  $n$ , vs. wavelength in microns,  $\lambda$ , was fit to an equation similar to that of Sellmeier:

$$n(\lambda) = \{a + b/(\lambda^2 - c)\}^{1/2}$$

The resulting best-fit equation was used to find the refractive index at the highest energy data points in our experimental spectra. For Tetraglyme, the results were

$$\begin{aligned} n(7800\text{ cm}^{-1}) &= 1.4139 \text{ at } 25\text{ }^{\circ}\text{C} \text{ for MIR data and} \\ n(10,000\text{ cm}^{-1}) &= 1.4178 \text{ at } 25\text{ }^{\circ}\text{C} \text{ for NIR and merged data.} \end{aligned}$$

### Post Processing and Related Parameters:

For the MIR, a composite spectrum was created from 7 absorbance spectra (base-10) taken at 7 path lengths: 3.70, 7.21, 19.8, 41.8, 112, 198 and 502 micrometers ( $\mu\text{m}$ ). For the NIR, a composite spectrum was created from 5 absorbance spectra (base-10) taken at 5 path lengths: 113, 200, 504, 990 and 3054  $\mu\text{m}$ . The same cells for the ~100, 200 and 500  $\mu\text{m}$  path lengths were used for both spectral ranges. At each path length several spectra were measured and the results averaged for better signal to noise. The measured cell lengths were adjusted using Beer's law plots in which the NIR and MIR data were analyzed independently.

- 1) The imaginary part of the refractive index, or  $k$  vector, was determined for each absorbance file as per Bertie's program "RNJ46A" (see reference above). This takes into account the reflective losses due to the KBr windows and the measured refractive index at 7800  $\text{cm}^{-1}$  for the MIR data and 10,000  $\text{cm}^{-1}$  for the NIR data.
- 2) A composite  $k$  vector is created via a classical, weighted, linear, least squares fit using the output files of program "RNJ46A": Intercept=0, slope is fitted, individual absorbance values weighted by  $T^2$  (transmission squared), all absorbance values  $\geq 2.5$  are given zero weight. For the MIR, four composite vectors were created and merged by hand.
  - a) The first  $k$  vector used the results from the 112 through 502  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 7800 to 4600  $\text{cm}^{-1}$  and 700 to 400  $\text{cm}^{-1}$ .
  - b) The second  $k$  vector used the results from the 42 through 198  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 4600 to 3300  $\text{cm}^{-1}$  and 2700 to 1550  $\text{cm}^{-1}$ .
  - c) The third  $k$  vector used the results from the 4 through 42  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 3300 to 2700  $\text{cm}^{-1}$ .
  - d) The fourth  $k$  vector used the results from the 4 through 112  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 1550 to 700  $\text{cm}^{-1}$ .
- 3) A frequency correction was applied to the resulting composite MIR  $k$  vector.
  - a) Frequency correction (already applied):  $\tilde{\nu}(\text{corrected}) = [\tilde{\nu}(\text{instrument}) * .999848 + .010722]$  as determined by comparing measured atmospheric spectral lines ( $\text{H}_2\text{O}$  and  $\text{CO}_2$ ) to values from the Northwest Infrared Spectral Library Database.
- 4) For the NIR, two composite vectors were created and merged by hand.
  - a) The first  $k$  vector used the results from the 990 and 3054  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 10,000 to 7500  $\text{cm}^{-1}$ .
  - b) The second  $k$  vector used the results from the 113 through 3054  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 7500 to 2000  $\text{cm}^{-1}$ .
- 5) A frequency correction was applied to the resulting composite NIR  $k$  vector.
  - a) Frequency correction (already applied):  $\tilde{\nu}(\text{corrected}) = [\tilde{\nu}(\text{instrument}) * .99987 + .00008278]$  as determined by comparing measured atmospheric spectral lines ( $\text{H}_2\text{O}$  and  $\text{CO}_2$ ) to values from the Northwest Infrared Spectral Library Database.
- 6) Finally, the MIR data were mapped onto the NIR x-axis using an interpolation routine, i.e. the Make Compatible command in OPUS 5.5. Then the composite MIR and NIR  $k$  vectors were merged to generate a final composite  $k$  vector across the entire spectral range. The NIR data were used exclusively above 5500  $\text{cm}^{-1}$ , and only the MIR data were used below 5100  $\text{cm}^{-1}$ . A weighted average, with the weight of the MIR vector increasing linearly from 0 to 100% between 5500 and 5100  $\text{cm}^{-1}$  was used in the overlapping spectral region. The resulting composite  $k$  vector and the refractive index at 10,000  $\text{cm}^{-1}$  were used to create the final  $n$  vector using the Kramers-Kronig relation, as per Bertie's program "LZZKTB."

### Photograph of Sample Tetraglyme:



Figure 2: Tetraglyme (Tetraethylene glycol dimethyl ether) in Aldrich container.